


Recommendations for preparing illustrations for the «Sechenov Medical Journal»


In the settings of the programme you use to view CT, MRI, etc. images, **please always look for the parameters of the maximum possible output image size.**

4 steps to download images with maximum resolution and size from RadiAnt DICOM:


STEP 1.

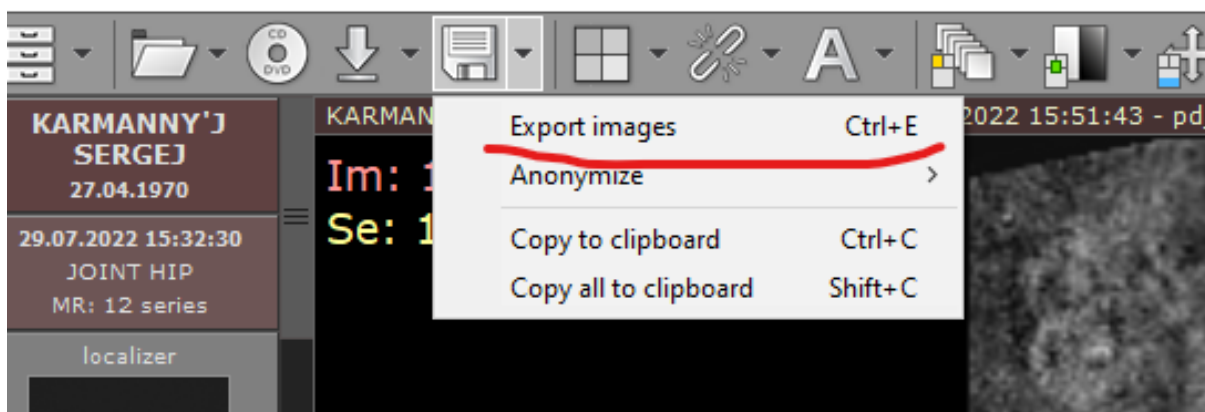

STEP 2

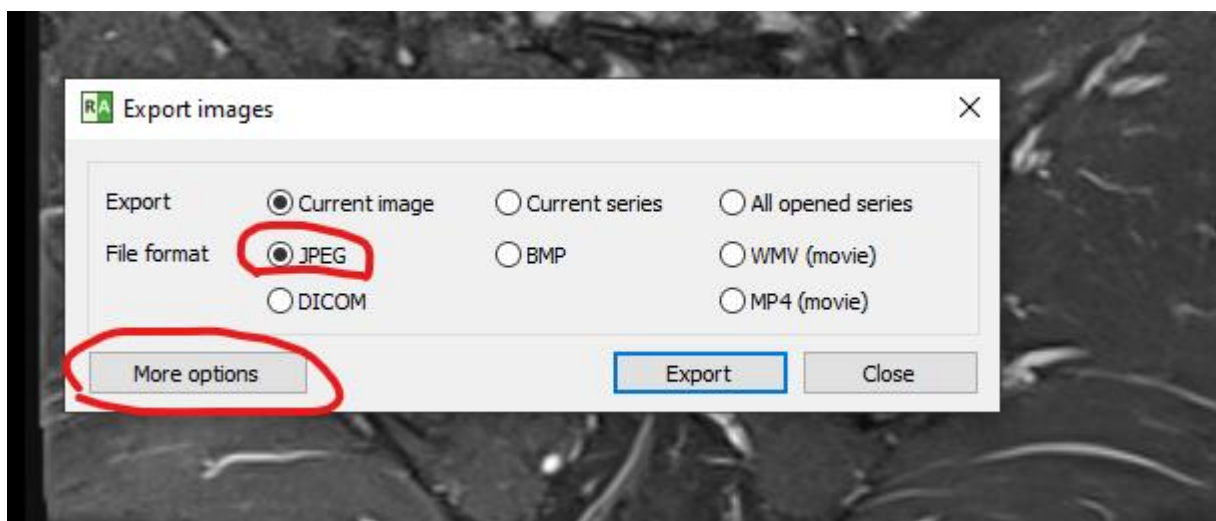

STEP 3

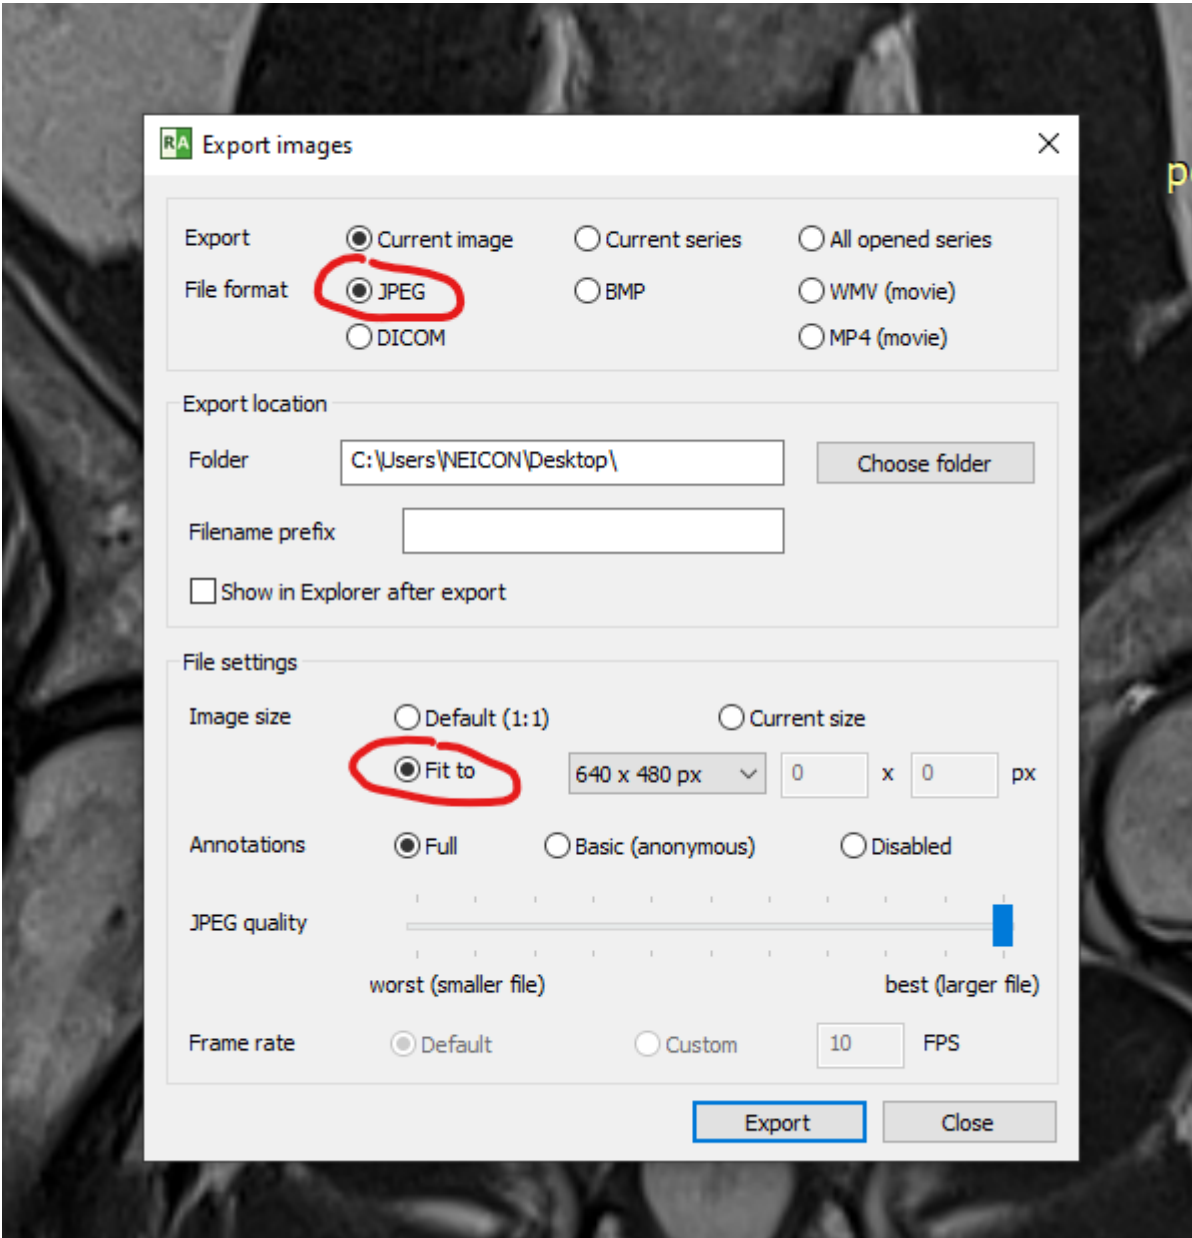

STEP 4

